

Mascarilla Quirúrgica Infantil (BFE \geq 98%)
De 6 a 9 años




Mascarilla Quirúrgica Infantil. Tipo IIR (BFE \geq 99%)

De 6 a 9 años



Información técnica

Tipología: Mascarilla quirúrgica infantil. Tipo IIR.
Desechable
Estándar: CE: EN 14683-2019 + AC:2019
Tamaño: 150 x 65 mm (6-9 años)
Eficacia de filtración bacteriana: \geq 99%
Prestaciones: resistente a salpicaduras
Estructura: cuerpo de la máscara, pinza nasal y agarre de la máscara
Caducidad: 24 meses
Aviso de alergia: Textil no tejido
Unidades / paquete: 10 unidades

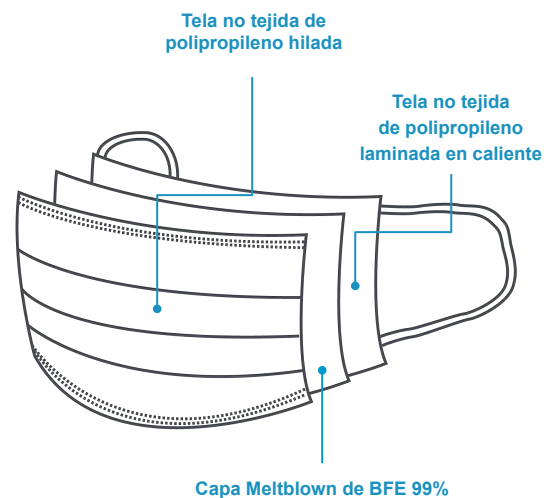

Instrucciones para ponerse la mascarilla

1. Con el lado azul hacia fuera, colóquela sobre la nariz y la boca. A continuación, pase las cintas por detrás de las orejas.
2. Presione suavemente el clip nasal para adaptarlo a la nariz.
3. Tire de la parte inferior de la mascarilla para que quede por debajo de la barbilla y compruebe el ajuste.



Información importante

- Material hipoalergénico, polipropileno y resistente al agua incluyendo la pinza nasal flexible.
- Informe de Ensayos CE emitido por TÜV SÜD.
- Condiciones de conservación: Almacenar en lugar con relativa baja humedad, libre de gases corrosivos, bien ventilado y evitando altas temperaturas ($>40^{\circ}\text{C}$).



Mascarilla Quirúrgica Infantil (BFE \geq 98%)
De 6 a 9 años



Mascarilla Quirúrgica Infantil. Tipo IIR (BFE \geq 98%)

De 6 a 9 años



CARACTERÍSTICAS	ESTÁNDAR	RESULTADOS
Bacterial Filtration Efficiency (BFE)	EN 14683:2019+AC:2019	BFE \geq 99%
Presión diferencial (ΔP)	EN 14683:2019+AC:2019	$\Delta P < 38$ Pa/cm ²
Limpieza Microbiana	EN 14683:2019+AC:2019	CFU/g < 20
Penetración de sangre sintética	ISO 22609:2004	No detectada

Fuente: Test Report No.: 200193327 (TÜV SÜD)

Características del paquete

Cantidad: 10 uds/paquete
SKU: MASK-ST-00025.0010
Dimensión: 215 x 115
Peso: 35 g

Características de la caja

Cantidad: 100 paquetes/caja
Total cantidad: 1.000 unidades
Dimensión: 500 x 370 x 230 mm





Certificados

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Declaración de conformidad



EU Declaration Of Conformity

Manufacturer **Diasia Biomedical Technology Co., Ltd.**
Address **3th B,4th Floor, Building No.4, Chuangfu Industrial Park, Xixiang Tiegang Reservoir Road, Baoan District, Shenzhen, China**
EC Representative **M/SCMC Medical Devices& Drugs S.L.**
C/ Horacio Lengo N° 18, CP 29006, Málaga, Spain
+34951214054

Product: **Disposable Medical Mask**

Model: **175mm×94mm , 145mm×94mm , 150mm×65mm**

Classification (MDD, Annex IX): **Class I Rule1**

We herewith declare that the above mentioned products meet the transposition into national law, The provisions of the following EC Council Directives and Standards. All supporting documentations are retained under the premises of the manufacturer. We are exclusively responsible for the DOC.

DIRECTIVES

General applicable directives:

Medical Device Directive: COUNCIL DIRECTIVE 93/42/EEC of 14 June 1993 concerning medical devices (MDD 93/42/EEC).

Standards:

EN 14683:2019;

ISO 10993-5:2009;

ISO 10993-10:2010;

All applicable harmonized standards (published in the Official Journal of the European Communities)

Date CE mark was affixed: **May 12, 2020**

Place, Date: **Shenzhen, 12.05.2020**

Signature: *Kirby Deng* General Manager

Name/Position: Kirby Deng / G.M.

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado


Produkte
Products



Prüfbericht-Nr.: Test Report No.:	60379483 001	Auftrags-Nr.: Order No.:	168265694	Seite 1 von 12 Page 1 of 12	
Kunden-Referenz-Nr.: Client Reference No.:	N/A	Auftragsdatum: Order date:	May 20, 2020		
Auftraggeber: Client:	Diasia Biomedical Technology Co., Ltd. 3th B, 4th Floor, Building No.4, Chuangfu Industrial Park, Xixiang Tiegang Reservoir Road, Baoan District, Shenzhen, China				
Prüfgegenstand: Test item:	Disposable Medical Mask				
Bezeichnung / Typ-Nr.: Identification / Type No.:	175mm x 94mm, 150mm x 65mm, 145mm x 94mm				
Auftrags-Inhalt: Order content:	Type test				
Prüfgrundlage: Test specification:	EN 14683:2019+AC:2019 except for clause 5.2.6				
Wareneingangsdatum: Date of receipt:	May 20, 2020	See Attachment: Photo documentation for details.			
Prüfmuster-Nr.: Test sample No.:	20200516				
Prüfzeitraum: Testing period:	May 21, 2020 to Jun. 01, 2020				
Ort der Prüfung: Place of testing:	See page 3				
Prüflaboratorium: Testing laboratory:	TÜV Rheinland (Shenzhen) Co., Ltd.				
Prüfergebnis*: Test result*:	Pass				
geprüft von / tested by:		kontrolliert von / reviewed by:			
 Jun. 28, 2020 Lucy Jiang / Assistant Project Engineer		 Jun. 28, 2020 Angela Chen / Department Manager			
Datum Date	Name / Stellung Name / Position	Unterschrift Signature	Datum Date	Name / Stellung Name / Position	Unterschrift Signature
Sonstiges / Other:					
- The test report consists of EN 14683 test report including this cover page (12 pages) and attachment: Photo documentation (9 pages). - The Biocompatibility (clause 5.2.6) is not evaluated in this test report.					
Zustand des Prüfgegenstandes bei Anlieferung: Condition of the test item at delivery:			Prüfmuster vollständig und unbeschädigt Test item complete and undamaged		
* Legende: 1 = sehr gut 2 = gut 3 = befriedigend 4 = ausreichend 5 = mangelhaft P(ass) = entspricht o.g. Prüfgrundlage(n) F(all) = entspricht nicht o.g. Prüfgrundlage(n) N/A = nicht anwendbar NT = nicht getestet Legend: 1 = very good 2 = good 3 = satisfactory 4 = sufficient 5 = poor P(ass) = passed a.m. test specification(s) F(all) = failed a.m. test specification(s) N/A = not applicable NT = not tested					
Dieser Prüfbericht bezieht sich nur auf das o.g. Prüfmuster und darf ohne Genehmigung der Prüfstelle nicht auszugsweise vervielfältigt werden. Dieser Bericht berechtigt nicht zur Verwendung eines Prüfzeichens. This test report only relates to the a. m. test sample. Without permission of the test center this test report is not permitted to be duplicated in extracts. This test report does not entitle to carry any test mark.					

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC: 2019 Medical face masks — Requirements and test methods	
Report Reference No.	60379483 001
Date of issue.....	See cover page
Total number of pages	See cover page
Testing Laboratory	TÜV Rheinland (Shenzhen) Co., Ltd.
Address.....	1F East & 2-4F, Cybio Technology Building No.1, No.16 Kejibei 2nd Road, High-Tech Industrial Park North Nanshan District, 518057, Shenzhen, China
Applicant's name	Diasia Biomedical Technology Co., Ltd.
Address.....	3th B, 4th Floor, Building No.4, Chuangfu Industrial Park, Xixiang Tiegang Reservoir Road, Baoan District, Shenzhen, China
Test specification:	
Standard	EN 14683:2019+AC:2019
Test procedure	Type test
Non-standard test method.....	N/A
Test Report Form No.	EN 14683:2019+AC:2019_A
Test Report Form Originator	TÜV Rh (SZ)
Master TRF	2020-03
Test item description.....	Disposable Medical Mask
Trade Mark.....	 — 德夏 —
Manufacturer	Same as the applicant
Model/Type reference.....	175mm × 94mm, 150mm × 65mm, 145mm × 94mm
Classification.....	Type IIR

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

List of Attachments (including a total number of pages in each attachment):	
Attachment – Photo Documentation (9 pages)	
Summary of testing:	
Tests performed (name of test and test clause): Construction check according to: Clause 5.1.1 Materials and construction Clause 5.1.2 Design	Testing location: TÜV Rheinland (Shenzhen) Co., Ltd. 1F East & 2-4F, Cybio Technology Building No.1, No.16 Kejibei 2nd Road, High-Tech Industrial Park North Nanshan District, 518057, Shenzhen, China
Clause 5.2.2 Bacterial filtration efficiency (BFE) Clause 5.2.3 Breathability Clause 5.2.4 Splash resistance Clause 5.2.5 Microbial cleanliness (Bioburden)	Pony Testing Group Shanghai Co., Ltd. 2/3/4/6/F., Building 35, No.680, Guiping Road, Xuhui District, Shanghai, China

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado



Page 4 of 12

Report No. 60379483 001

Copy of marking plate

The artwork below may be only a draft. The use of certification marks on a product must be authorized by the respective NCBs that own these marks.

See attachment.

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado



Page 5 of 12

Report No. 60379483 001

Testing
Date of receipt of test item(s): See cover page
Dates of tests performed: See cover page
Possible test case verdicts:
- test case does not apply to the test object: N/A
- test object does meet the requirement: P (Pass)
- test object was not evaluated for the requirement: N/E (collateral standards only)
- test object does not meet the requirement: F (Fail)
General remarks:
"(See Attachment #)" refers to additional information appended to the report. "(See appended table)" refers to a table appended to the report. The tests results presented in this report relate only to the object tested. This report shall not be reproduced except in full without the written approval of the testing laboratory. List of test equipment must be kept on file and available for review. Additional test data and/or information provided in the attachments to this report.
Throughout this report a <input type="checkbox"/> comma / <input checked="" type="checkbox"/> point is used as the decimal separator.
Name and address of factory (ies): Same as the applicant
General product information:
1, The tested medical mask classified as type IIR. 2, The Biocompatibility (clause 5.2.6) is not evaluated in this test report. 3, The test results are for reference only. Relevant certification may be needed if the mask is intended to be sold in Europe. 4, Three models are identical with each other except for the size, the sizes for three models are 175mm x 94mm, 150mm x 65mm and 145mm x 94mm. All the tests are performed on model 175mm x 94mm.

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC:2019			
Clause	Requirement + Test	Result - Remark	Verdict
4	Classification		P
	Medical face masks specified in this European Standard are classified into two types (Type I and Type II) according to bacterial filtration efficiency whereby Type II is further divided according to whether or not the mask is splash resistant. The 'R' signifies splash resistance.	Type IIR	P
5	Requirements		P
5.1	General		P
5.1.1	Materials and construction		P
	The medical face mask is a medical device, generally composed of a filter layer that is placed, bonded or moulded between layers of fabric.	3 ply designed with two layers of non-woven fabric and one layer of melt blown fabric.	P
	The medical face mask shall not disintegrate, split or tear during intended use.		P
	In the selection of the filter and layer materials, attention shall be paid to cleanliness.		P
5.1.2	Design		P
	The medical face mask shall have a means by which it can be fitted closely over the nose, mouth and chin of the wearer and which ensures that the mask fits closely at the sides.		P
	Medical face masks may have different shapes and constructions as well as additional features such as a face shield (to protect the wearer against splashes and droplets) with or without anti-fog function, or a nose bridge (to enhance fit by conforming to the nose contours).	With nose clip	P
5.2	Performance requirements		P
5.2.1	General		P
	All tests shall be carried out on finished products or samples cut from finished products.		P
5.2.2	Bacterial filtration efficiency (BFE)		P
	When tested in accordance with Annex B, the BFE of the medical face mask shall conform to the minimum value given for the relevant type in Table 1.	See appended table 5.2.2	P
	For thick and rigid masks such as rigid duckbill or cup masks the test method may not be suitable as a proper seal cannot be maintained in the cascade impactor. In these cases, another valid equivalent method shall be used to determine the BFE.	Not such mask.	N/A

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC:2019			
Clause	Requirement + Test	Result - Remark	Verdict
	When a mask consists of two or more areas with different characteristics or different layer-composition, each panel or area shall be tested individually.	Same characteristics and same layer-composition declared by manufacturer.	N/A
	The lowest performing panel or area shall determine the BFE value of the complete mask	See above	N/A
5.2.3	Breathability		P
	When tested in accordance with Annex C, the differential pressure of the medical face mask shall conform to the value given for the relevant type in Table 1.	See appended table 5.2.3	P
	If the use of a respiratory protective device as face mask is required in an operating theatre and/or other medical settings, it might not fulfil the performance requirements with regard to differential pressure as defined in this European Standard. In such case, the device should fulfil the requirement as specified in the relevant Personal Protective Equipment (PPE) standard(s).		N/A
5.2.4	Splash resistance		P
	When tested in accordance with ISO 22609:2004 the resistance of the medical face mask to penetration of splashes of liquid shall conform to the minimum value given for Type IIR in Table 1.	See appended table 5.2.4	P
5.2.5	Microbial cleanliness (Bioburden)		P
	When tested according to EN ISO 11737-1:2018 the bioburden of the medical mask shall be ≤ 30 CFU/g tested (see Table 1).	See appended table 5.2.5	P
5.2.6	Biocompatibility		N/E
	According to the definition and classification in EN ISO 10993-1:2009, a medical face mask is a surface device with limited contact.	The biocompatibility is not evaluated in this test report.	N/E
	The manufacturer shall complete the evaluation of the medical face mask according to EN ISO 10993-1:2009 and determine the applicable toxicology testing regime.		N/E
	The results of testing should be documented according to the applicable parts of the EN ISO 10993 series.		N/E
	The test results shall be available upon request.		N/E
6	Marking, labelling and packaging		P
	Annex I, §13, of the Medical Devices Directive (93/42/EEC) or Annex I, §23, of the Medical Device Regulation (EU) 2017/745 specifies the information that should be specified on the packaging in which the medical face mask is supplied.	See attachment.	P
	The following information shall be supplied:		P
	a) number of this European Standard;		P

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado



Page 8 of 12

Report No. 60379483 001

EN 14683:2019+AC:2019

Clause	Requirement + Test	Result - Remark	Verdict
	b) type of mask (as indicated in Table 1).		P
	EN ISO 15223-1:2016 and EN 1041:2008+A1:2013 should be considered.		P

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC:2019								
Clause	Requirement + Test				Result - Remark			Verdict
5.2.2		TABLE: Bacterial filtration efficiency (BFE)						P
Batch/ lot no.:	Test Specimen no.:	Dimension of the test specimen L x W (mm x mm)	test area (cm ²)	Flow rate (l/min)	Mean of the total plate counts of the two positive controls	Mean plate count of the negative controls	BFE for each test specimen (%)	Remarks
2020051 6	1	164×144	95.0	28.3	1729	0	99.4	--
	2	164×145	95.0	28.3			99.8	--
	3	163×144	95.0	28.3			99.6	--
	4	164×144	95.0	28.3			99.6	--
	5	165×145	95.0	28.3			99.8	--
Supplementary information:								
1, Each specimen was conditioned at 21 °C and 85 % relative humidity for 4 h to bring them into equilibrium with atmosphere prior to testing.								
2, The side of the test specimen was facing towards the challenge aerosol: <u>the inside of the test specimen.</u>								

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC:2019					
Clause	Requirement + Test			Result - Remark	Verdict
5.2.3	TABLE: Breathability (Differential pressure)				P
Batch/ lot no.:	Test Specimen number- Test area number	Differential pressure for each test area (Pa/cm ²)	The averaged differential pressure for each test specimen (Pa/cm ²)	Flow rate (l/min)	Remarks
202005 16	1-1	26.2	26.9	8.0	--
	1-2	28.2		8.0	--
	1-3	26.9		8.0	--
	1-4	28.1		8.0	--
	1-5	25.1		8.0	--
	2-1	32.0	32.2	8.0	--
	2-2	31.9		8.0	--
	2-3	32.9		8.0	--
	2-4	31.3		8.0	--
	2-5	33.1		8.0	--
	3-1	29.6	29.2	8.0	--
	3-2	27.9		8.0	--
	3-3	30.3		8.0	--
	3-4	27.6		8.0	--
	3-5	30.7		8.0	--
	4-1	31.9	32.3	8.0	--
	4-2	33.4		8.0	--
	4-3	31.8		8.0	--
	4-4	31.1		8.0	--
	4-5	33.2		8.0	--
	5-1	31.8	31.8	8.0	--
	5-2	32.3		8.0	--
	5-3	29.9		8.0	--
	5-4	33.0		8.0	--
	5-5	31.9		8.0	--
Supplementary information:					
Each specimen was conditioned at 21 °C and 85 % relative humidity for 4 h to bring them into equilibrium with					

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado

EN 14683:2019+AC:2019

Clause	Requirement + Test	Result - Remark	Verdict
	atmosphere prior to testing.		

5.2.4		TABLE: Splash resistance			P
Batch/ lot no.:	Test mask no.:	The material of tested mask	Test result (Pass/fail)	Remarks	
20200516	1	See clause 5.1.1	Pass	--	
	2		Pass	--	
	3		Pass	--	
	4		Pass	--	
	5		Pass	--	
	6		Pass	--	
	7		Pass	--	
	8		Pass	--	
	9		Pass	--	
	10		Pass	--	
	11		Pass	--	
	12		Pass	--	
	13		Pass	--	
	14		Pass	--	
	15		Pass	--	
	16		Pass	--	
	17		Pass	--	
	18		Pass	--	
	19		Pass	--	
	20		Pass	--	
	21		Pass	--	
	22		Pass	--	
	23		Pass	--	
	24		Pass	--	
	25		Pass	--	
	26		Pass	--	
	27		Pass	--	
	28		Pass	--	

Mascarilla Quirúrgica / Quirúrgica Infantil BFE 99%

Certificado



Page 12 of 12

Report No. 60379483 001

EN 14683:2019+AC:2019				
Clause	Requirement + Test		Result - Remark	Verdict
	29		Pass	--
	30		Pass	--
	31		Pass	--
	32		Pass	--

Supplementary information:
 1, Each specimen was conditioned at 21 °C and 85 % relative humidity for 4 h to bring them into equilibrium with atmosphere prior to testing.
 2, The description of target area tested: the centre of the specimen.
 3, Any technique used to enhance visual detection of synthetic blood: cotton absorbent swab.
 4, The temperature and relative humidity for testing: 21 °C and 85 %.
 5, Description of any pre-treatment techniques used: N/A.

5.2.5	TABLE: Microbial cleanliness (Bioburden)				P
Batch/ lot no.:	Mask(under test) no.:	Weight of each mask (g)	Total bioburden per individual mask (CFU/g)	Remarks	
20200516	1	3.00	19	--	
	2	3.01	15	--	
	3	3.01	25	--	
	4	2.99	21	--	
	5	3.00	16	--	

Supplementary information:

End of EN 14683 test report